


**Lampiran 9. Hasil Uji Kadar Betakaroten**

15/04/19 16:56

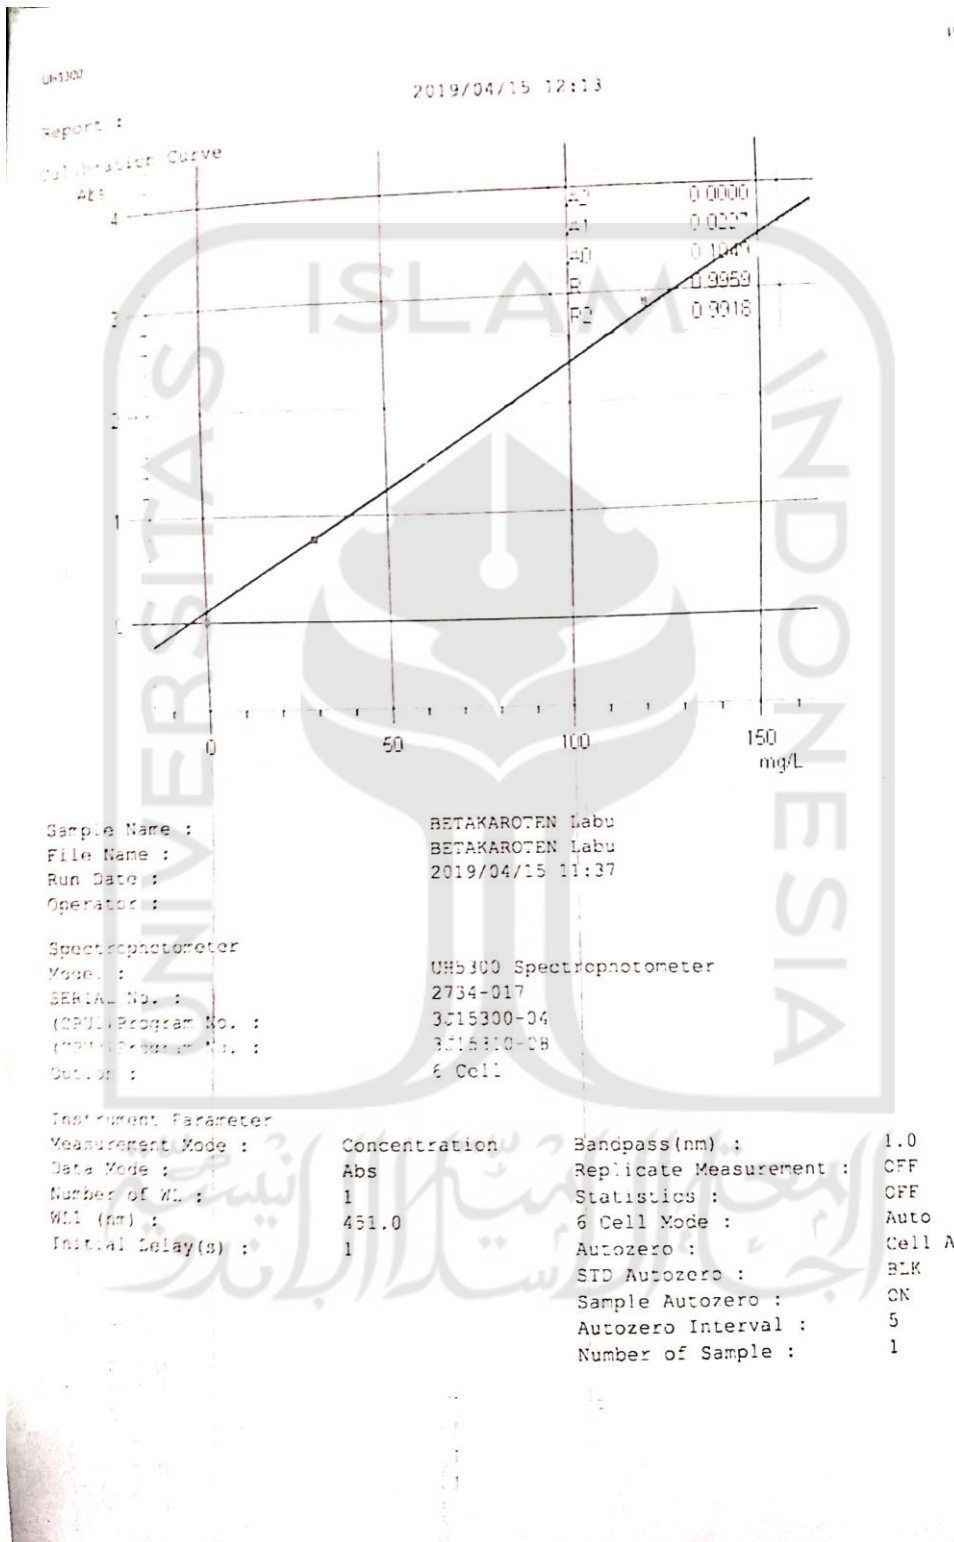

043700

STD	Abn	CONC (mg/L)	DIFF	RD	T
STD1	0.001	0.0000	-4.5712	-253.36073	-0.89790
STD2	0.174	10.0000	-0.3096	-17.16039	-0.06082
STD3	1.131	60.0000	2.9628	164.23372	0.58197
STD4	2.279	90.0000	5.9726	331.03503	1.17317
STD5	2.698	120.0000	3.2608	180.73399	0.64651
STD6	3.338	150.0000	-7.3154	-405.46162	-1.43694

Curve Information  
 Calibration Curve Type : 1st Order  
 Calibration Curve Formula : Abs=f(CONC)  
 Through Zero : OFF  
 CONC Min : 0.0000  
 CONC Max : 100.0000  
 Calibration Curve Factor : A0 : 0.1049 A1 : 0.0227  
 Factor : Correlation Coefficient: R =0.9959  
 Determination Coefficient: R2 =0.9918

Sample

Sample No	Abn	CONC (mg/L)
TP 0	2.805	119.1706 H
24 JAM 0	2.678	113.5737 H
36 JAM 0	2.699	114.5113 H
48 JAM 0	3.286	140.3812 H
TP 0	2.626	111.2719 H
24 JAM 0	2.683	113.8057 H
36 JAM 0	2.603	110.2569 H
48 JAM 0	2.785	118.3009 H

UNIVERSITAS PADJARAN  
 INDONESIA  
 الجامعة الإسلامية في اندونيسيا